



Creating a method based on standard parameter

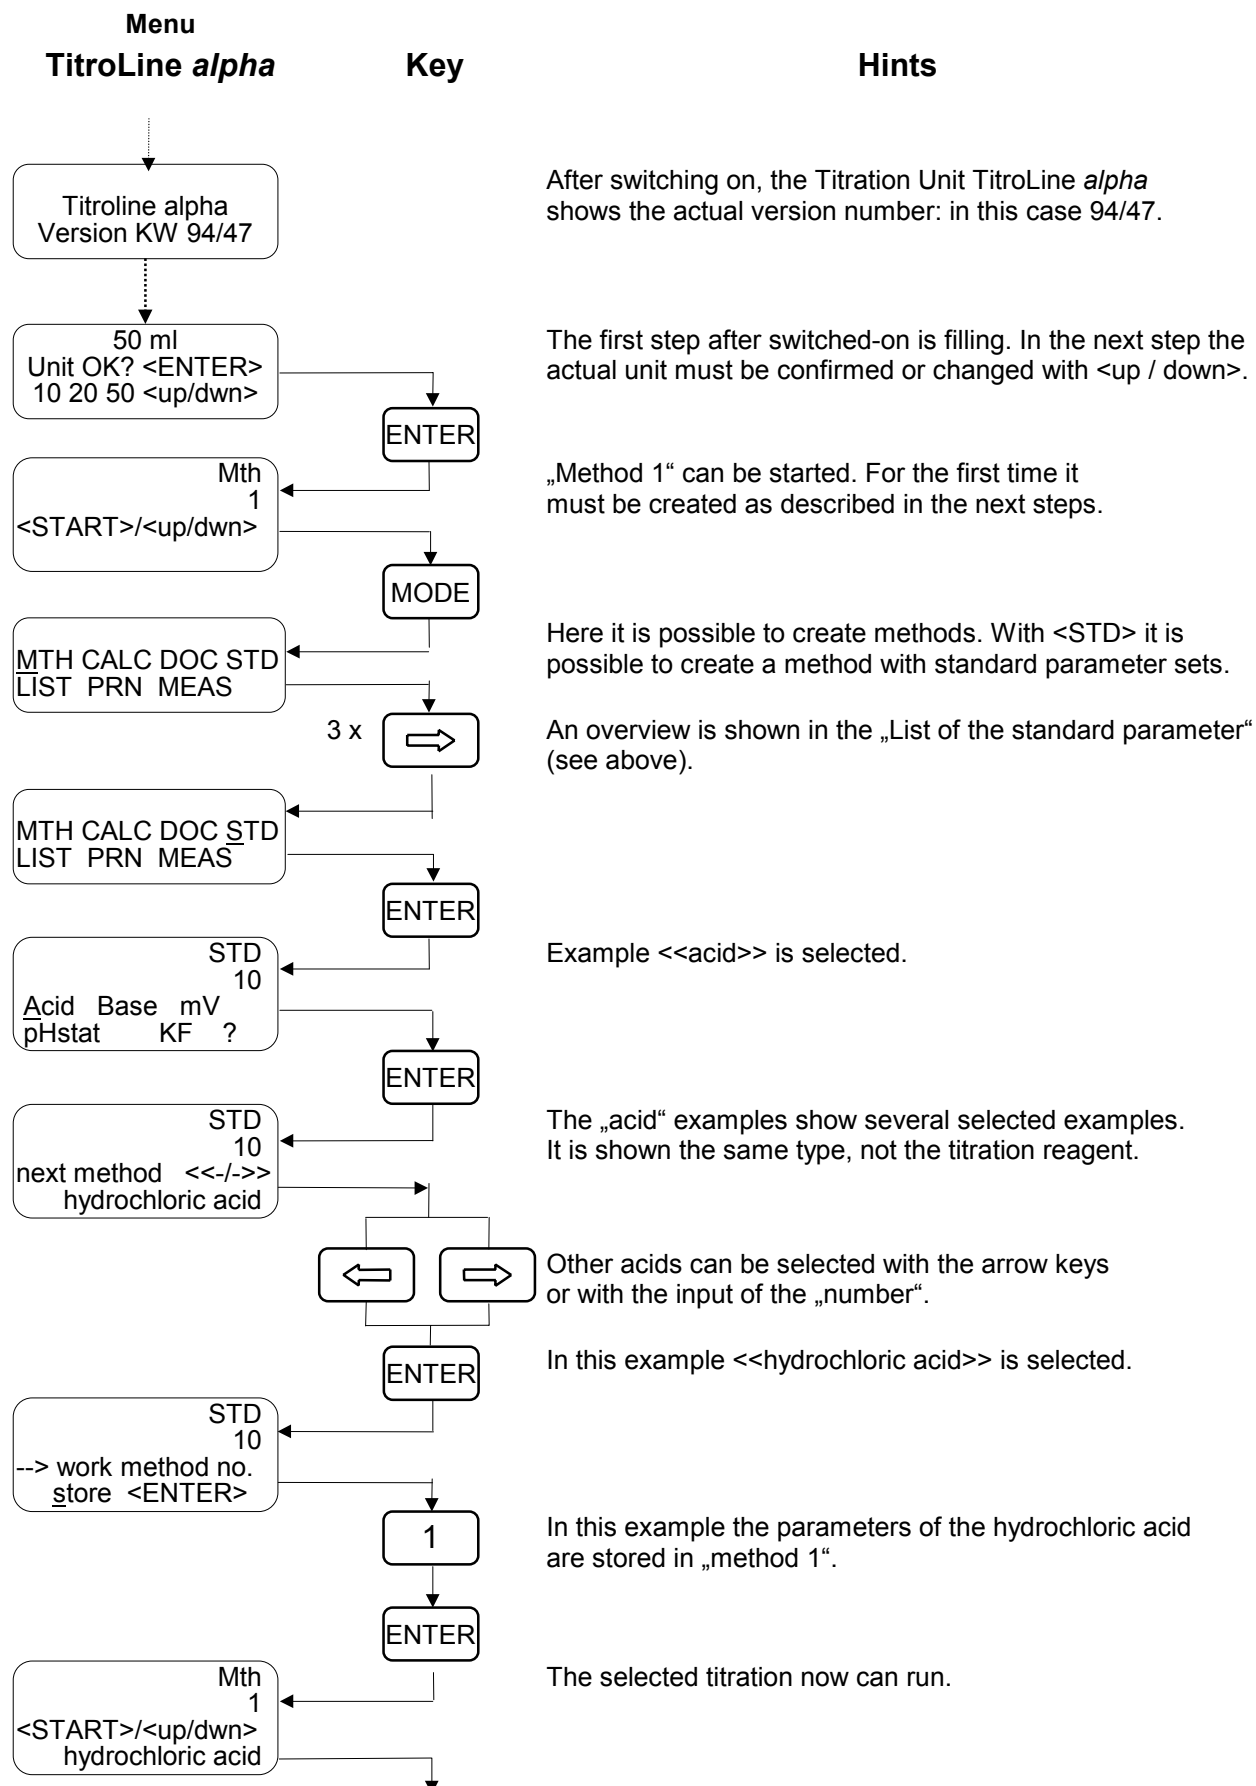

Creating a method based on standard parameter

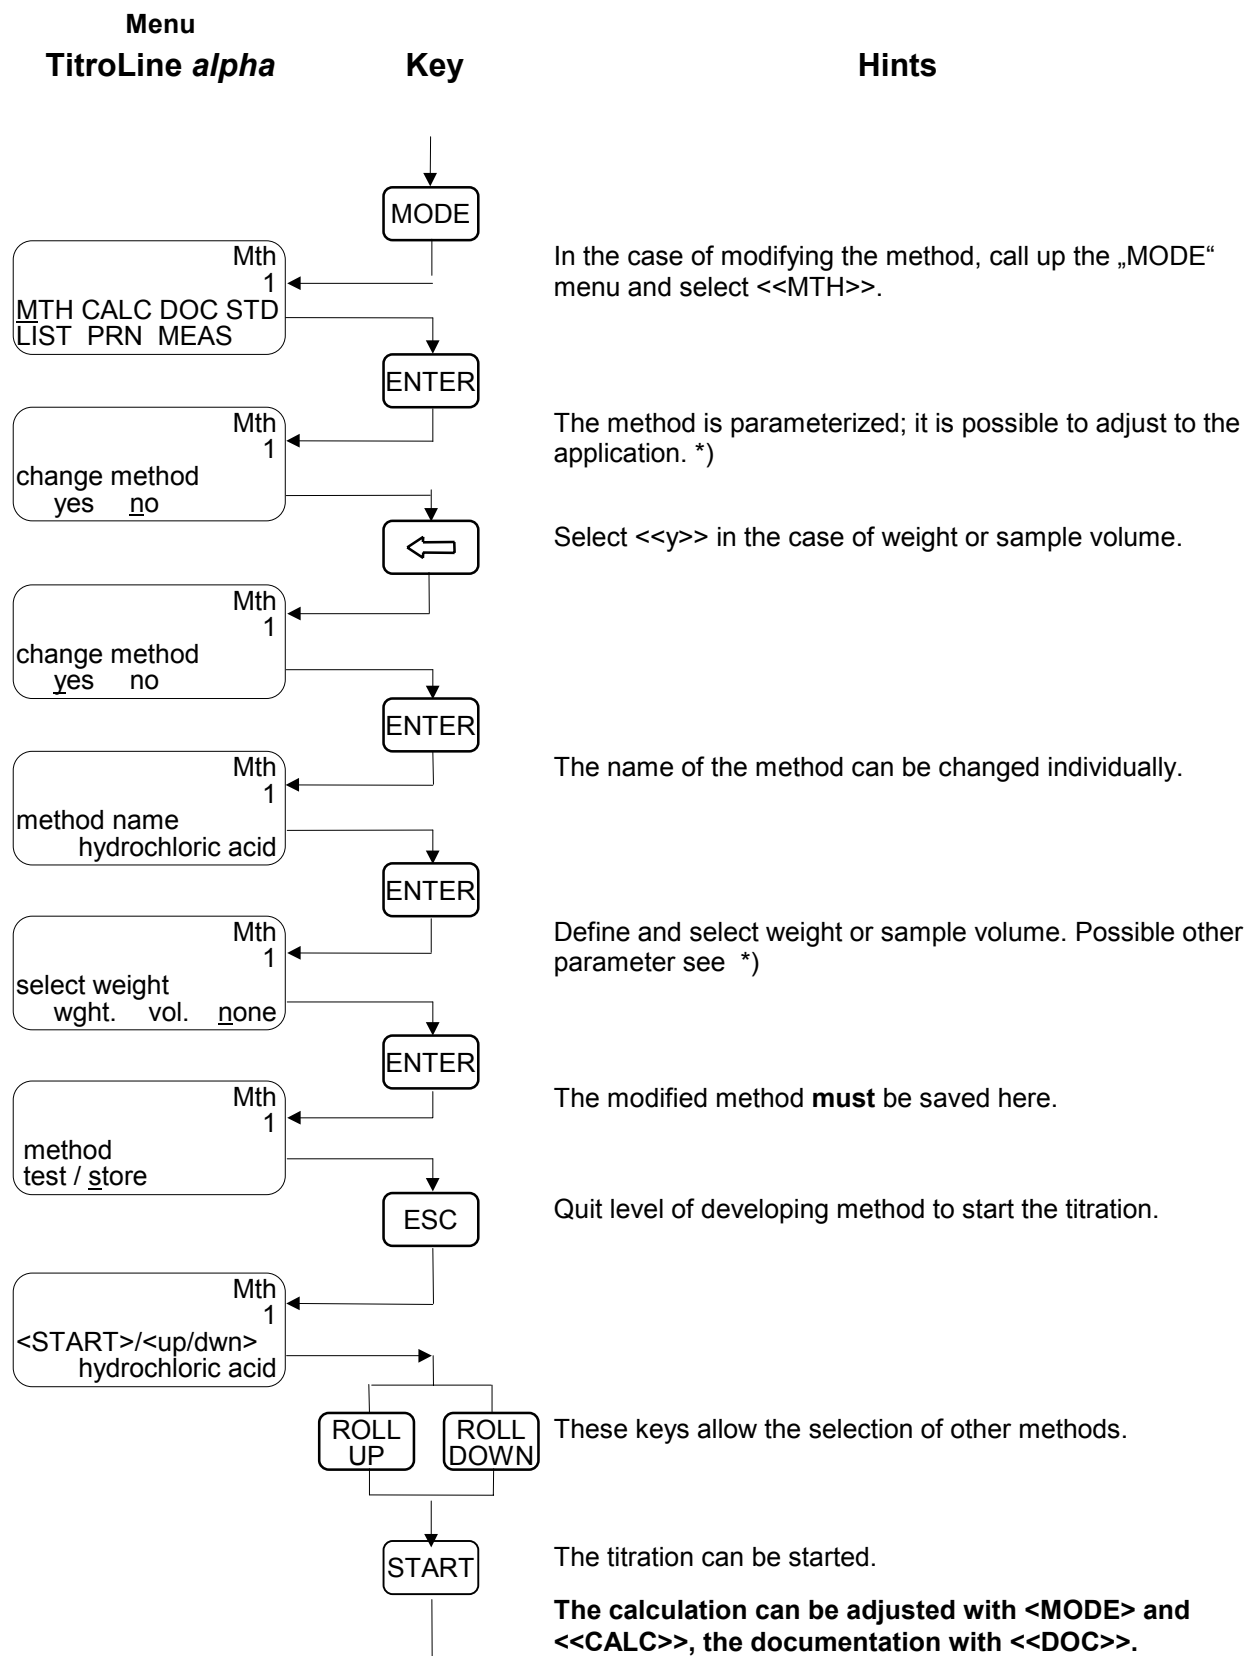

*) In the menu <INIT> you must switch on the menu point „editing standard parameters“ in <SYS> in the case you want to change the predefined titration parameters. Then it is possible to change the parameters.

